


April 30, 2019

Dear Healthcare Professional,
cc: Chairman Medical Board and relevant Head of Departments

Subject: URGENT MEDICAL DEVICE RECALL

Affected Product: Oxford Unicompartmental Knee Drill Guides (Phase 3/Domed Lateral)

Item Number	Lot Number	Item Description	Item Number	Lot Number	Item Description
32-420321	ZB160201	Phase 3 Femoral Drill Guide Small	32-420323	ZB170301	Phase 3 Femoral Drill Guide Large
32-420321	ZB160401		32-420323	ZB170401	
32-420321	ZB161101		32-420323	ZB170901	
32-420321	ZB170401		32-420324	ZB110301	Phase 3 Femoral Drill Guide Extra Large
32-420321	ZB170601		32-421060	ZB160601	Phase 3 Femoral Drill Guide Extra Small
32-420321	ZB170801		32-421060	ZB170201	
32-420321	ZB170901		32-421060	ZB170601	
32-420322	ZB130801	Phase 3 Femoral Drill Guide Medium	32-421930	ZB160101	System Domed Lateral Femoral Drill Guide Small
32-420323	ZB161102	Phase 3 Femoral Drill Guide Large	32-421930	ZB160801	
32-420323	ZB170201		32-421931	ZB150901	System Domed Lateral Femoral Drill Guide Medium

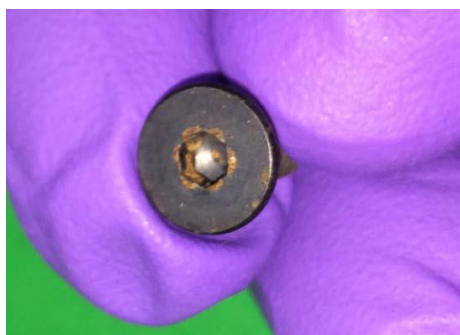

Zimmer Biomet is conducting a lot specific medical device recall for the Oxford Unicompartmental Knee Drill Guides (Phase 3/Domed Lateral) due to the incorrect raw material used by the supplier in the manufacturing of the screw component, which material could potentially lead to corrosion.

Risks		
Describe immediate health consequences (injuries or illness) that may result from use of or exposure to the product issue.	Most Probable	Highest Severity
	<i>None – alternative device obtained and used.</i>	<i>Device used and corrosion identified during surgery – extension to surgery > 30 minutes to obtain new device.</i>
Describe long range health consequences (injuries or illness) that may result from use of or exposure to the product issue.	Most Probable	Highest Severity
	<i>None – alternative device obtained and used.</i>	<i>Adverse tissue reaction/inflammatory response due to foreign debris. Potential revision surgery required as a result.</i>

Our records indicate that you may have received one or more of the affected products. The affected units were distributed between March 2016 and August 2018.

Risk Manager Responsibilities:

1. Review this notification and ensure that affected personnel are aware of the contents.
2. If you have affected product at your facility, assist your Zimmer Biomet sales representative and quarantine all affected product. Your Zimmer Biomet sales representative will remove the affected product from your facility.
3. Complete **Attachment 1 – Certificate of Acknowledgement** and send to CorporateQuality.PostMarket@zimmerbiomet.com. This form must be returned even if you do not have affected products at your facility.
4. Retain a copy of the acknowledgement form with your recall records in the event of a compliance audit of your facility's documentation.
5. If you have further questions or concerns after reviewing this notice, please call customer service at 574-371-3071 between 8:00 am and 5:00pm EST, Monday through Friday. Calls received outside of call center operating hours will receive a voicemail prompt or be transferred to an on-call representative in the event of an emergency. Alternatively, your questions may be emailed to CorporateQuality.PostMarket@zimmerbiomet.com.

Other Information

This medical device recall was reported to the U.S. Food and Drug Administration and will be reported to other Competent Authorities, Notified Bodies, and Regulatory Authorities as required.

- Med Watch Reporting: Adverse reactions or quality problems experienced with the use of this product may be reported to the FDA's Med Watch Adverse Event Reporting program either online, by mail, or by fax.
- Online: www.fda.gov/medwatch/report.htm
- Mail: Use postage paid, pre-addressed form FDA 3500, available at: www.fda.gov/MedWatch/getforms.htm
- Fax: 1-800-FDA-0178



Under 21 CFR 803, manufacturers are required to report any serious injuries where a product has contributed or may have contributed to the event. Please keep Zimmer Biomet informed of any adverse events associated with this product or any other Zimmer Biomet product by emailing product.experience@zimmerbiomet.com.

Please be aware that the names of user facilities notified are routinely provided to the Competent Authorities for audit purposes. The undersigned confirms that this notice has been delivered to the appropriate Regulatory Agencies.

Thank you for your assistance. We regret any inconvenience caused by this recall.

Sincerely,



Kevin W. Escapule
Post Market Surveillance and Regulatory Compliance Director

ATTACHMENT 1

Certificate of Acknowledgement

IMMEDIATE RESPONSE REQUIRED – TIME SENSITIVE ACTION NEEDED

Affected Product: Oxford Unicompartmental Knee Drill Guides (Phase 3/Domed Lateral)

Field Action Reference: ZFA 2018-00529

Do you have affected product in your facility?

(Hospital Facility Only: Please mark the appropriate response.)

- ☐ **Yes**, we currently have one or more affected items in our facility.
- ☐ **No**, we currently have no affected items in our facility.

By signing below, I acknowledge that the required actions have been taken in accordance with this recall notice.

Printed Name: _____ **Signature:** _____

Title: _____ **Telephone:** () _____ - _____ **Date:** ____/____/____

Facility Name: _____

Facility Address: _____

City: _____ **State:** _____ **ZIP:** _____

Note: This form must be returned to Zimmer Biomet before this action is closed for your account. It is important that you complete this form and email a copy to CorporateQuality.PostMarket@zimmerbiomet.com or fax to 574-373-3589.